

## Ordering Information

### AMPLATZER Septal Occluder

Model / Reorder Number	Waist Diameter (mm)	Waist Width (mm)	Right Atrial Disc Diameter (mm)	Left Atrial Disc Diameter (mm)
9-ASD-004	4	3	12	16
9-ASD-005	5	3	13	17
9-ASD-006	6	3	14	18
9-ASD-007	7	3	15	19
9-ASD-008	8	3	16	20
9-ASD-009	9	3	17	21
9-ASD-010	10	3	18	22
9-ASD-011	11	4	21	25
9-ASD-012	12	4	22	26
9-ASD-013	13	4	23	27
9-ASD-014	14	4	24	28
9-ASD-015	15	4	25	29
9-ASD-016	16	4	26	30
9-ASD-017	17	4	27	31
9-ASD-018	18	4	28	32
9-ASD-019	19	4	29	33
9-ASD-020	20	4	30	34
9-ASD-022	22	4	32	36
9-ASD-024	24	4	34	38
9-ASD-026	26	4	36	40
9-ASD-028	28	4	38	42
9-ASD-030	30	4	40	44
9-ASD-032	32	4	42	46
9-ASD-034	34	4	44	50
9-ASD-036	36	4	46	52
9-ASD-038	38	4	48	54
9-ASD-040 <sup>a</sup>	40	4	50	56

### AMPLATZER Cribriform Occluder

Model / Reorder Number	Right & Left Atrium Disc Diameter (mm)	Waist Width (mm)
9-ASD-MF-018	18	3
9-ASD-MF-025	25	3
9-ASD-MF-030	30	3
9-ASD-MF-035	35	3
9-ASD-MF-040 <sup>a</sup>	40	3

a. Device not available in all markets. Device not available the United States.

#### References

1. AMPLATZER Septal Occluder Instructions for Use.
2. Kashour TS, Latroche B, Elhoury ME, et. al. Successful Percutaneous Closure of a Secundum Atrial Septal Defect through Femoral Approach in a Patient with Interrupted Inferior Vena Cava. *Congenital Heart Disease*. 2010;5(6):620-623.

ATRIAL FIBRILLATION    CARDIAC RHYTHM MANAGEMENT    CARDIOVASCULAR    NEUROMODULATION

#### Global Headquarters

One St. Jude Medical Drive  
St. Paul, Minnesota 55117  
USA  
+1 651 756 2000  
+1 651 756 3301 Fax

#### Cardiovascular Division

177 East County Road B  
St. Paul, Minnesota 55117  
USA  
+1 651 756 4470  
+1 651 756 4466 Fax

#### Amplatzer Products

5050 Nathan Lane North  
Plymouth, Minnesota 55442  
USA  
+1 763 513 9227  
+1 763 513 9226 Fax

#### US Division

6300 Bee Cave Road  
Building Two, Suite 100  
Austin, Texas 78746  
USA  
+1 512 732 7400  
+1 512 732 2418 Fax

#### St. Jude Medical Coordination Center BVBA

The Corporate Village  
Avenue Da Vincilaan 11 Box F1  
B-1935 Zaventem  
Belgium  
+32 2 774 68 11  
+32 2 772 83 84 Fax

#### St. Jude Medical Japan Co., Ltd.

Shiodome City Center 15F  
1-5-2, Higashi-Shinbashi  
Minato-ku  
Tokyo 105 7115  
Japan  
+81 3 6255 6370  
+81 3 6255 6371 Fax

#### St. Jude Medical (Hong Kong) Ltd.

Suite 1608, 16/F Exchange Tower  
33 Wang Chiu Road  
Kowloon Bay, Kowloon  
Hong Kong SAR  
+852 2996 7688  
+852 2956 0622 Fax

#### St. Jude Medical Brasil Ltda.

Rua Frei Caneca, 1380  
7º ao 9º andares  
01307-002 - São Paulo (SP)  
Brazil  
+55 11 5080 5400  
+55 11 5080 5423 Fax

[SJMprofessional.com](http://SJMprofessional.com)



#### Rx Only

**Brief Summary:** Please review the Instructions for Use prior to using these devices for a complete listing of indications, contraindications, warnings, precautions, potential adverse events, and directions for use.

ST. JUDE MEDICAL, the nine-squares symbol and MORE CONTROL. LESS RISK. are trademarks and service marks of St. Jude Medical, Inc. and its related companies. ©2011 St. Jude Medical. All rights reserved.

MM00236 (06) Global 07/11

## AMPLATZER™ Septal Occluders Structural Heart Therapy



# THE PROVEN STANDARD FOR TRANSCATHETER ATRIAL SEPTAL DEFECT CLOSURE<sup>1, 2</sup>

AMPLATZER Septal Occluders are the standard of care for minimally invasive atrial septal defect (ASD) closure. These double-disc occluders are comprised of Nitinol mesh with polyester fabric. They are designed to appose the septal wall on each side of the defect and create a platform for tissue in-growth after implantation.

## When Simplicity Matters

The primary treatment option for closure of secundum atrial septal defects is with transcatheter devices.<sup>2</sup> This is when trust and simplicity matter.

The AMPLATZER Septal Occluder is the proven standard of care in transcatheter ASD closure.<sup>1, 2</sup>

### SAFETY IN NUMBERS

**98.5% Closure Rate:** With no significant residual shunt (less than 2 mm) at 1-year follow-up<sup>1</sup>

### Low Major and Minor Complication Rates:

Post-procedure and long-term based on 5-year follow-up<sup>1</sup>


### SPECIFICALLY DESIGNED FOR ASD CLOSURE

**Wide Waist:** Centers device and fills the ASD

**Shape-memory Nitinol Mesh:** Designed to securely appose both sides of the septal wall

**Polyester Material:** Promotes occlusion and tissue in-growth

**Precise Placement:** Device can be easily recaptured and redeployed

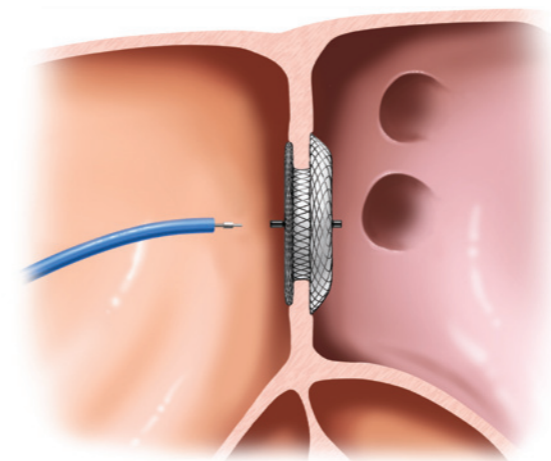

The waist of the AMPLATZER Septal Occluder fills the defect for optimal occlusion.

## When Flexibility Matters

Not all septal defects are the same. They come in a variety of shapes, sizes and often there can be multiple communications between the left and right atria. These types of atrial septal defects require a special device designed with the flexibility to meet multiple needs.

The addition of the AMPLATZER Multit-Fenestrated Septal Occluder - "Cribriform" to the AMPLATZER family of occluders enables transcatheter closure for the majority of atrial septal defects.


### SPECIFICALLY DESIGNED FOR MULTI-FENESTRATED ASD CLOSURE

**Narrow Waist:** Allows for placement through a central defect

**Matched Disc Diameters:** Maximizes coverage of multiple fenestrations

**Polyester Material:** Promotes occlusion and tissue in-growth

**Precise Placement:** Device can be easily recaptured and redeployed

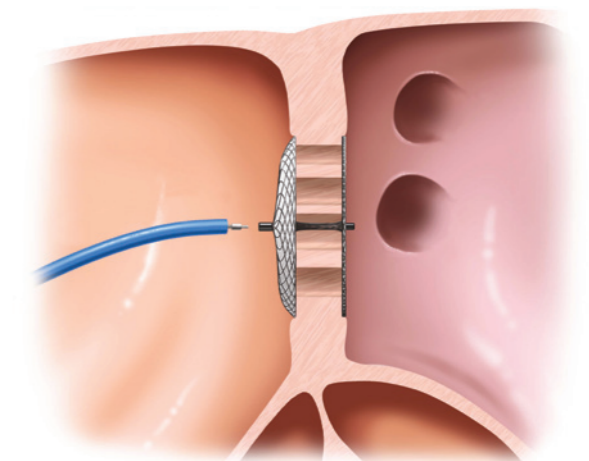

The AMPLATZER Cribriform Occluder enables occlusion of the defect by covering the fenestrations with a single device.

Stocking both AMPLATZER Septal and Cribriform Occluders provides you the ability to choose the appropriate device for a wide size-range of defects.